


-15kV TOF: -9245 v
 -3.6kV MCP: -3364 v
 -2.4kV MCP: -1774 v
 Input Cur: 314 ma
 RPA max: 237 v
 Mirror max: 167 v

Wed Nov 15 10:37:43 2006

TIDE Direct Events

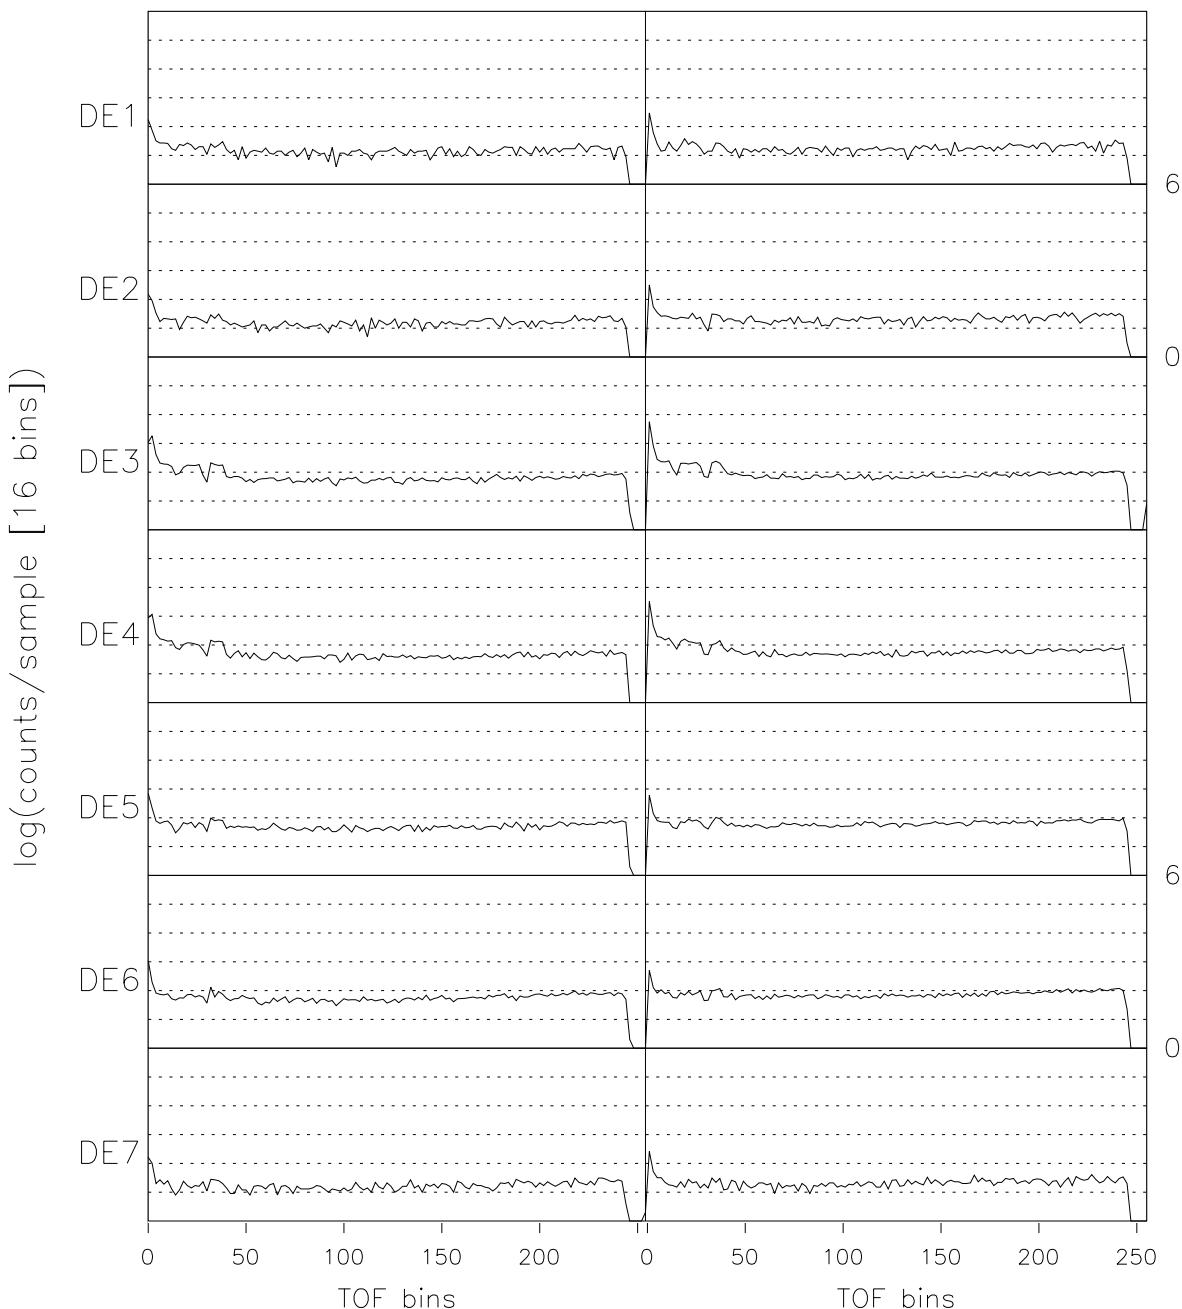

reported: 10-12-06 17:11:19 UT

reported: 10-12-06 17:14:32 UT

file: /export/data/tide/nrt/06101201.dat

-15kV TOF: -9181 v
-3.6kV MCP: -3364 v
-2.4kV MCP: -1774 v
Input Cur: 296 ma
RPA max: 237 v
Mirror max: 238 v